

► GIOVANNA IEZZI, ANTONIO SCARANO, VITTORIA PERROTTI, DOMENICO TRIPODI, ADRIANO PIATTELLI

Department of Medical, Oral and Biotechnological Sciences, Dental School, University of Chieti-Pescara, Chieti, Italy

Immediately loaded blade implants. A histological and histomorphometrical evaluation after a long loading period. A retrospective 20 years analysis (1989-2009)

TO CITE THIS ARTICLE

Iezzi G, Scarano A, Perrotti V, Tripodi D, Piattelli A. Immediately loaded blade implants. A histological and histomorphometrical evaluation after a long loading period. A retrospective 20 years analysis (1989-2009). *J Osseointegr* 2012;3(4):39-42.

ABSTRACT

Aim Although the presence of mineralized tissues at the interface with blade implants has been reported, the view that blade implants cannot integrate still persists. Blades are the immediately loaded implants with the longest clinical history, so their histological evaluation may give results applicable to root-form implants. The aim of the present retrospective study was a histological evaluation of the peri-implant tissues in immediately loaded human blade implants retrieved after a long loading history.

Materials and methods Thirty-one implants were included in the present report, after a loading history varying from 2 to 23 years, with a mean of 15 years. The implants were processed for histological examination.

Results Histologically, the bone was in close and tight contact with the implants surface and no gaps or connective fibrous tissues were present at the implant-bone interface. The peri-implant bone was compact, mature, with the presence of small marrow spaces and Haversian canals. Many osteons were in contact with the implant surface. Most Haversian systems ran perpendicular to the major axis of the blades. In some fields it was possible to observe the presence of a few osteoblasts. Remodelling areas were present. Mean bone to implant contact percentage was, for all 31 implants, $43 \pm 5.2\%$.

Conclusion The present report showed that immediately loaded blade implants can achieve and maintain osseointegration under long-term function (more than 20 years).

KEY WORDS Blade implants; Bone-implant interface; Immediately loaded implants; Retrieved human implants.

INTRODUCTION

Blade implants have been reported to have a lower survival rate, attributed to the formation of connective tissues around the implants (1). The presence of mineralized tissues at the interface with blade implants has already been reported (1-5); however, the view that blade implants cannot integrate still persists (1). Very high success and survival rates have been reported in immediately loaded dental root-form implants (6-11), and immediately loaded implants have shown a clinical long-term predictability similar to those of conventionally loaded implants (12, 13). Immediate loading determines an instant reduction of the oral handicap and shortens the total treatment time with increased patient satisfaction, decreased patient anxiety and discomfort, better function and esthetics, and avoidance of a conventional denture during the healing period (12, 14). When primary stability is achieved, and a proper prosthetic treatment plan is followed, immediate loading is a feasible concept (13).

Many clinicians probably are not aware that the concept of immediate loading was proposed more than 40 years ago when the endosseous blade implants were introduced (15). Histological evidence of osseointegration in clinically successfully osseointegrated implants in man can be found in the literature (16-35). Retrieved human implants are extremely important for long-term evaluation of implants subjected to functional loading (1-5). Blades are the immediately loaded implants with the longest clinical history, so their histological evaluation has an historical value and may certainly have some applications to root-form implants (1).

The aim of the present retrospective study was a histological evaluation of the peri-implant tissues in immediately loaded human blade implants retrieved after a long loading history.

MATERIALS AND METHODS

The archives of the Implant Retrieval Center of the

Dental School of the University of Chieti-Pescara, Chieti, Italy, were retrospectively searched (1989–2009) to look for retrieved human blade implants. The clinical and laboratory records were evaluated carefully, and only the blade implants that complied to the following inclusion criteria were analysed.

- 1) Presence of healthy peri-implant soft tissues, with no bleeding on probing.
- 2) Absence of mobility.
- 3) Absence of pain upon percussion.
- 4) No signs of bone or soft tissue pathology present during implant retrieval.
- 5) Absence of a peri-implant radiolucency and radiographical presence of mineralized tissues.
- 6) Fabrication and insertion of an interim implant-supported prosthesis on the day of implant surgery.

Out of 85 retrieved blade implants found, only 31 met all the inclusion criteria. Only these 31 implants were part of the present report, while the others were discarded. These 31 implants had been retrieved for different causes, mainly for a fracture of the abutment, for a fracture of the prosthesis or due to changes in the prosthetic rehabilitation of the patients, after a loading history varying from 2 to 23 years, with a mean of 15 years.

All the implants had been retrieved with a bur under abundant saline irrigation.



FIG. 1 Clinical view of a removed blade; hard tissues are present in direct contact with the implant.

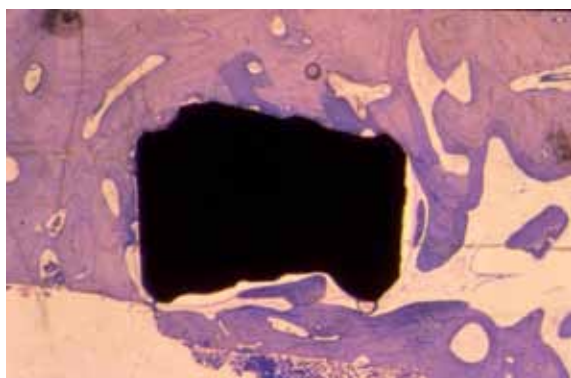


FIG. 2 At low magnification, it was possible to observe mineralized bone with the presence of small marrow spaces and Haversian canals in contact with the implant surface. Acid fuchsin-toluidine blue 50X.

Processing of specimens

The implants and the surrounding tissues were stored immediately in 10% buffered formalin and processed to obtain thin ground sections with the Precise 1 Automated System (36).

The specimens were dehydrated in an ascending series of alcohol rinses and embedded in a glycolmethacrylate resin. After polymerization the specimens were sectioned longitudinally along the major axis of the implants with a high-precision diamond disc at about 150 μ m and ground down to about 30 μ m. Three slides were obtained for each implant. The slides were stained with basic fuchsin and toluidine blue. A double staining with von Kossa and acid fuchsin was done to evaluate the degree of bone mineralization, and one slide, after polishing, was immersed in AgNO₃ for thirty minutes, and exposed to sunlight; the slides were then washed under tap water, dried and immersed in basic fuchsin for five minutes, and then washed and mounted.

Histomorphometry of bone-implant contact percentage was carried out using a light microscope connected to a high resolution videocamera and interfaced to a monitor and PC. This optical system was associated with a digitizing pad and a histometry software package with image capturing capabilities.

RESULTS

All 31 implants were lined by mineralized tissues (Fig. 1). At low magnification, it was possible to observe mineralized bone in contact with the implant surface (Fig. 2). The bone was in close and tight contact with the implants surface and no gaps or connective fibrous tissues were present at the implant-bone interface. In some areas of the bone interface, an artefact was present because bone had been removed during the retrieval procedure. The peri-implant bone was compact, mature, with the presence of small marrow spaces and Haversian canals (Fig. 3). Some osteons were present

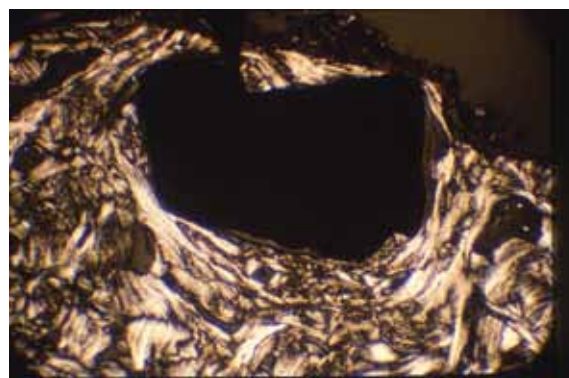


FIG. 3 Some osteons were present near the metal surface; each osteon was composed by a Haversian system and about 10 to 20 bone lamellae. Acid fuchsin-toluidine blue 50X. Polarized light.

near the metal surface; each osteon was composed by a Haversian system and about 10 to 20 bone lamellae. Most Haversian systems ran perpendicular to the major axis of the blade. In some fields it was possible to observe the presence of a few osteoblasts.

Remodeling areas were present (Fig. 4). Near some of the implants the bone lamellae tended to run parallel to the implant surfaces.

The newly-formed bone was more strongly stained with acid fuchsin and it was clearly separated from the old, pre-existing bone (Fig. 5).

No inflammatory infiltrate was present. No epithelial downgrowth was present. In the areas of remodelling bone it was possible to observe bone remodelling units with vessels, osteoblasts and osteoclasts. Lamellar and woven bone were separated by a well-defined irregular cement line. Some of the marrow spaces abutted on the implant surface and some of the Haversian systems were in direct contact with the implant surface.

Mean bone to implant contact percentage was for all 31 implants $43 \pm 5.2\%$.

DISCUSSION AND CONCLUSION

Healing processes are strongly influenced by the local mechanical loading history (37). Mechanical loading of the skeleton regulates the attainment of peak bone mass in the growing animal and produces adaptive changes in the adult (38). An immediate loading protocol implies healing under loading and involves the risk of fibrous tissue encapsulation (39).

Histological examination provides the best evidence of the type of tissue at the interface with dental implants. Only rarely the histology of human retrieved immediately loaded implants have been reported in the literature (16-22, 30, 33). Even more rarely it is possible to find histological reports in the literature of immediately loaded implants with a long-term follow-up (1-3, 5, 24-26). The presence of mineralized tissues

at the interface with blade implants, even after a long loading history, has already been reported (1-3).

In blade implants retrieved after 13 and 21 years of function, mature bone in tight contact with the implant surface was seen around most of the implant surface (1). In another report, about 40% of the blade implant interface was lined by mineralized tissue (4).

The present histological data showed that mineralized tissues were present at the interface with immediately loaded blade implants and that these tissues were successfully maintained over a very long time period (in some cases more than 20 years).

The response of the bone tissue appeared not to be disturbed by the stresses and strains transmitted at the interface. Minimal lateral forces exerted on the implants have been reported to be critical factors for success. Probably, the precise, intimate fit of the implants in the bone, obtained by a bone hole smaller than the implant diameter, was helpful in obtaining mineralized tissues at the interface. It has been reported that controlled implant micromotion had a positive effect on the bone formation at the interface (37).

The present histological results could be explained by the fact that functional loading appears to stimulate bone apposition (40-44). Wolff stated that there was a direct link between mechanical loading and bone form; Wolff's law would imply that increased stresses acted as a stimulus to new bone formation while reduced stress tended to produce bone loss (41-44).

In conclusion, the present report showed that immediately loaded blade implants can achieve and maintain osseointegration even under long-term function (more than 20 years).

ACKNOWLEDGMENTS

This work was partially supported by the National Research Council (C.N.R.), Rome, Italy, by the Ministry of Education, University, Research (M.I.U.R.), Rome, Italy.

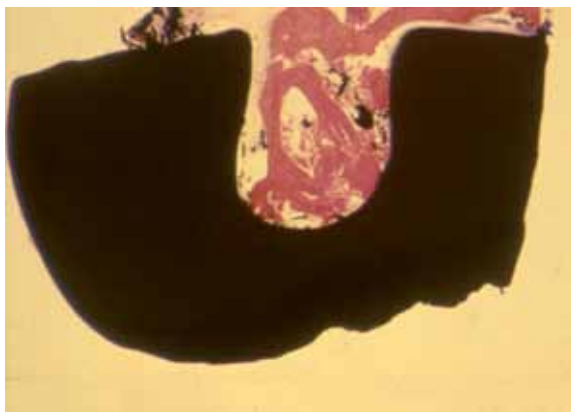


FIG. 4 Trabecular bone with large osteocyte lacunae is present in direct contact with the implant surface. Acid fuchsin-toluidine blue 50X.

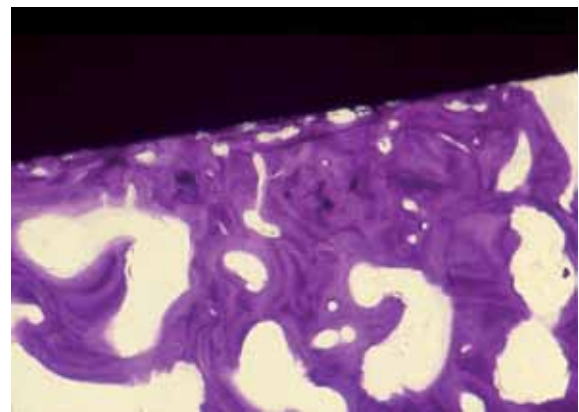


FIG. 5 Remodeling areas are present. A large osteocyte lacuna is present. Acid fuchsin-toluidine blue 50X.

REFERENCES

- Prousaefs P, Lozada J. Evaluation of two Vitallium blade-form implants retrieved after 13 and 21 years of function: a clinical report. *J Prosthet Dent* 2002;87:412-415.
- Trisi P, Emanuelli M, Quaranta M, Piattelli A. A Light Microscopy, Scanning Electron Microscopy and Laser Scanning Microscopy Analysis of retrieved blade implants after 7 to 20 years of clinical function. *J Periodontol* 1993;64:374-378.
- DiStefano D, Iezzi G, Scarano A, Perrotti V, Piattelli A. Immediately loaded blade implant retrieved from man after a 20 years loading period: a histological and histomorphometrical case report. *J Oral Implantol* 2006;32:171-176.
- Steflik DE, Sisk AL, Parr GR et al. Correlative transmission electron microscopic and scanning electron microscopic observations of the tissue supporting endosteal blade implants. *J Oral Implantol* 1992;18:110-120.
- Linkow LI, Donath K, Lemons JE. Retrieval analyses of a blade implant after 231 months of clinical function. *Implant Dent* 1992;1:37-43.
- Horiuchi K, Uchida H, Yamamoto K, Sugimura M. Immediate loading of Branemark system implants following placement in edentulous patients: a clinical report. *Int J Oral Maxillofac Implants* 2000;15:824-830.
- Jaffin RA, Kumar A, Berman CL. Immediate loading of implants in partially and fully edentulous jaws: a series of 27 case reports. *J Periodontol* 2000;71:833-838.
- Ganeles SJ, Rosenberg MM, Holt RL, Reichman LH. Immediate loading of implants with fixed restorations in the completely edentulous mandible: report of 27 patients from a private practice. *Int J Oral Maxillofac Implants* 2001;16:418-426.
- Degidi M, Piattelli A. Immediate functional and non functional loading of dental implants: a 2 to 60 months follow-up study of 646 titanium implants. *J Periodontol* 2003;74:225-241.
- Prousaefs P, Lozada J. Immediate loading of hydroxyapatite-coated implants in the maxillary premolar area: three-year results of a pilot study. *J Prosthet Dent* 2004;91:228-233.
- Glauser R, Lundgren AK, Gottlow J et al. Immediate occlusal loading of Branemark TiUniteTM implants placed predominantly in soft bone: 1-year results of a prospective clinical study. *Clin Impl Dent Relat Res* 2003;5(suppl.1):47-56.
- Lekholm U. Immediate/early loading of oral implants in compromised patients. *Periodontology* 2000 2003;33:194-203.
- Gapski R, Wang HL, Mascarenhas P, Lang NP. Critical review of immediate implant loading. *Clin Oral Impl Res* 2003;14:515-527.
- Laviv A, Levin L, Schwartz-Arad D. Survival of immediately provisionized dental implants: a case-control study with up to 5 years follow-up. *Clin Impl Dent Relat Res* (in press).
- Linkow LI, Miller RJ. Immediate loading of endosseous implants is not new. *J Oral Implantol* 2004;30:314-317.
- Testori T, Szmukler-Moncler S, Francetti L et al. Immediate loading of Osseotite implants. A case report and histologic analysis after 4 months of occlusal loading. *Int J Periodontics and Restorative Dent* 2001;21:451-459.
- Rocci A, Martignoni M, Miranda Burgos P, Gottlow J, Sennerby L. Histology of retrieved immediately and early loaded oxidized implants: light microscopic observations after 5 to 9 months of loading in the posterior mandible. *Clin Impl Dent Relat Res* 2003;5(Suppl.1):88-98.
- Degidi M, Petrone G, Iezzi G, Piattelli A. Histologic evaluation of 2 human immediately loaded and 1 submerged titanium implants inserted in the posterior mandible and retrieved after 6 months. *J Oral Implantol* 2003;29:223-229.
- Testori T, Szmukler-Moncler S, Francetti L, Del Fabbro M, Trisi P, Weinstein RL. Healing of Osseotite implants under submerged and immediate loading conditions in a single patient: a case report and interface analysis after 2 months. *Int J Periodontics Restorative Dent* 2002;22:345-353.
- Degidi M, Petrone G, Iezzi G, Piattelli A. Histologic evaluation of a human immediately loaded titanium implant with a porous anodized surface. *Clin Implant Dent Relat Res* 2002;4:110-114.
- Degidi M, Scarano A, Petrone G, Piattelli A. Histological analysis of clinically retrieved immediately loaded implants: a report of 11 cases. *Clin Impl Dent Relat Res* 2003;5:89-94.
- Degidi M, Scarano A, Iezzi G, Piattelli A. Peri-implant bone in immediately loaded titanium implants: an histologic and histomorphometric evaluation in man. A report of 2 cases. *Clin Impl Dent Relat Res* 2003;5:170-175.
- Romanos GE. Present status of immediate loading of oral implants. *J Oral Implantol* 2004;30:189-197.
- Prousaefs P. Histologic evaluation of an immediately loaded titanium provisional implant retrieved after functioning for 18 months: a clinical report. *J Prosthet Dent* 2003;89:331-334.
- Ledermann PD, Schenk RK, Buser D. Long-lasting osseointegration of immediately loaded bar-connected TPS screws after 12 years of function: a histologic case report of a 95-year-old patient. *Int J Periodontics Restorative Dent* 1998;18:558-563.
- Piattelli A, Scarano A, Paolantonio M. Immediately loaded screw implant removed for fracture after a 15-year loading period: histological and histochemical analysis. *J Oral Implantol* 1997;23:75-79.
- Traini T, Neugebauer J, Thams U, Zoeller, Caputi S, Piattelli A. Peri-implant bone organization under immediate loading conditions: collagen fibers orientation and mineral density analyses in the minipig model. *Clin Implant Dent Relat Res* 2009;11:41-51.
- Degidi M, Nardi D, Piattelli A. Immediate rehabilitation of the edentulous mandible with a definitive prosthesis supported by an intra-oral welded titanium bar. *Int J Oral Maxillofac Implants* 2009;24:342-347.
- Degidi M, Nardi D, Piattelli A. Immediate restoration of small-diameter implants in cases of partial posterior edentulism: a 4-year case series. *J Periodontol* 2009;80:1006-1012.
- Barros RRM, Degidi M, Novaes AB Jr, Piattelli A, Shibli JA, Iezzi G. Osteocyte density in the peri-implant bone of immediately loaded and submerged dental implants. *J Periodontol* 2009;80:499-504.
- Degidi M, Piattelli A, Shibli JA, Perrotti V, Iezzi G. Early bone formation around immediately restored implants with and without occlusal contact: a histologic and histomorphometric evaluation in man. A case report. *Int J Oral Maxillofac Implants* 2009;24:734-739.
- Degidi M, Nardi D, Piattelli A. Immediate vs one-stage restoration of small diameter implants for a single missing maxillary lateral incisor: a three-year randomized clinical trial. *J Periodontol* 2009;80:1393-1398.
- Degidi M, Piattelli A, Shibli JA, Perrotti V, Iezzi G. Bone formation after 4 and 8 weeks around immediately loaded and submerged dental implants with a modified sandblasted and acid-etched surface. A histologic and histomorphometric analysis in man. *Int J Oral Maxillofac Implants* 2009;24:896-901.
- Neugebauer J, Iezzi G, Perrotti V et al. Experimental immediate loading in conjunction with grafting procedures. *J Biomed Mater Res Part B Appl Biomater* 2009;91B:604-612.
- Degidi M, Iezzi G, Perrotti V, Piattelli A. Comparative analysis of immediate functional loading and immediate non-functional loading to traditional healing periods: a five-year follow-up of 550 dental implants. *Clin Impl Dent Relat Res* 2009;11:257-266.
- Piattelli A, Scarano A, Quaranta M. High-precision, cost-effective system for producing thin sections of oral tissues containing dental implants. *Biomaterials* 1997;18:577-579.
- Vandamme K, Naert I, Geris L, Vander Sloten J, Puers R, Duyck J. Histodynamics of bone tissue formation around immediately loaded cylindrical implants in the rabbit. *Clin Oral Impl Res* 2007;18:471-480.
- Fritton JC, Myers ER, Wright TM, van der Meulen MCH. Loading induces site-specific increases in mineral content assessed by micro-computed tomography of the mouse tibia. *Bone* 2005;36:1030-1038.
- Vandamme K, Naert I, Vander Sloten J, Puers R, Duyck J. Effect of implant surface roughness and loading on peri-implant bone formation. *J Periodontol* 2008;79:150-157.
- Donath K. Tissue reactions around loaded and unloaded titanium implants. *J Hard Tissue Biol* 1993;2:37-47.
- Frost HM. Wolff's law and bone's structural adaptations to mechanical usage: an overview for clinicians. *Angle Orthod* 1994;64:175-188.
- Frost HM. Bone "mass" and the "mechanostat": a proposal. *Anat Rec* 1987;219:1-9.
- Forwood MR, Turner CH. Skeletal adaptations to mechanical usage: results from tibial loading studies in rats. *Bone* 1995;17:197s-205s.
- Cowin SC. Wolff's law of trabecular architecture at remodeling equilibrium. *J Biomech Eng* 1986;108:83-88.